

INTERNATIONAL
STANDARD

ISO
16840-11

First edition
2022-05

**Wheelchair seating —
Part 11:
Determination of dissipation
characteristics of sensible
perspiration into seat cushions**

STANDARDSISO.COM : Click to view the full PDF of ISO 16840-11:2022



Reference number
ISO 16840-11:2022(E)

© ISO 2022

STANDARDSISO.COM : Click to view the full PDF of ISO 16840-11:2022



COPYRIGHT PROTECTED DOCUMENT

© ISO 2022

All rights reserved. Unless otherwise specified, or required in the context of its implementation, no part of this publication may be reproduced or utilized otherwise in any form or by any means, electronic or mechanical, including photocopying, or posting on the internet or an intranet, without prior written permission. Permission can be requested from either ISO at the address below or ISO's member body in the country of the requester.

ISO copyright office
CP 401 • Ch. de Blandonnet 8
CH-1214 Vernier, Geneva
Phone: +41 22 749 01 11
Email: copyright@iso.org
Website: www.iso.org

Published in Switzerland

Contents

	Page
Foreword	iv
Introduction	v
1 Scope	1
2 Normative references	1
3 Terms and definitions	1
4 Abbreviated terms	2
5 Principle	2
6 Test apparatus	2
6.1 Perspiration rigid cushion loading indenter	2
6.1.1 Shape of PRCLI	2
6.1.2 Temperature control on the PRCLI	2
6.1.3 Loading mechanism	3
6.1.4 Discharge mechanism	3
6.1.5 Sensing system	4
6.2 Electrical impedance measurement system	4
6.3 Test environment	4
7 Preparation for testing	5
8 Test method	5
9 Test report	5
Bibliography	8

STANDARDSISO.COM : Click to view the full PDF of ISO 16840-11:2022

Foreword

ISO (the International Organization for Standardization) is a worldwide federation of national standards bodies (ISO member bodies). The work of preparing International Standards is normally carried out through ISO technical committees. Each member body interested in a subject for which a technical committee has been established has the right to be represented on that committee. International organizations, governmental and non-governmental, in liaison with ISO, also take part in the work. ISO collaborates closely with the International Electrotechnical Commission (IEC) on all matters of electrotechnical standardization.

The procedures used to develop this document and those intended for its further maintenance are described in the ISO/IEC Directives, Part 1. In particular, the different approval criteria needed for the different types of ISO documents should be noted. This document was drafted in accordance with the editorial rules of the ISO/IEC Directives, Part 2 (see www.iso.org/directives).

Attention is drawn to the possibility that some of the elements of this document may be the subject of patent rights. ISO shall not be held responsible for identifying any or all such patent rights. Details of any patent rights identified during the development of the document will be in the Introduction and/or on the ISO list of patent declarations received (see www.iso.org/patents).

Any trade name used in this document is information given for the convenience of users and does not constitute an endorsement.

For an explanation of the voluntary nature of standards, the meaning of ISO specific terms and expressions related to conformity assessment, as well as information about ISO's adherence to the World Trade Organization (WTO) principles in the Technical Barriers to Trade (TBT), see www.iso.org/iso/foreword.html.

This document was prepared by Technical Committee ISO/TC 173, *Assistive products*, Subcommittee SC 1, *Wheelchairs*.

This first edition of ISO 16840-11 cancels and replaces ISO/TS 16840-11:2014, which has been technically revised.

The main changes are as follows:

- addition of details around the test apparatus, preparation and method to make the test easier to process.

A list of all parts in the ISO 16840 series can be found on the ISO website.

Any feedback or questions on this document should be directed to the user's national standards body. A complete listing of these bodies can be found at www.iso.org/members.html.

Introduction

Dissipating perspiration and moisture on seat cushions is important to prevent pressure injuries and tissue maceration, and for comfortable sitting. Perspiration can occur as water vapour, and/or as moisture – sensible moisture has not undergone a phase change to vapour, whereas insensible moisture has undergone the phase change and is in the vapour phase.

The results of the testing methods in this document have not been clinically validated to support any medical claims of prevention of pressure injuries or prevention of tissue maceration.

STANDARDSISO.COM : Click to view the full PDF of ISO 16840-11:2022

STANDARDSISO.COM : Click to view the full PDF of ISO 16840-11:2022

Wheelchair seating —

Part 11:

Determination of dissipation characteristics of sensible perspiration into seat cushions

1 Scope

This document specifies a method for determining the dissipation characteristics of simulated sensible perspiration exposure on seat cushions of a wheelchair under test conditions that simulate body loading on support surfaces with flat and contoured profiles. The test method is applicable to a wide variety of seat cushion materials and constructions that are used across the world.

The test method is intended to determine how the cushion handles a liquid load. It is not intended to determine how the cushion responds to a continuous release of liquid or vapour.

This document also specifies apparatus to measure dissipation characteristics (of perspiration) of seat cushions and the approach to be employed in measuring these characteristics.

This document is applicable to seat cushions for wheelchairs that include a cushion cover.

NOTE The significance of the dissipation characteristics of the seat cushion can be greatly affected by the clothing worn, for example a moisture wicking cover might not help the skin condition of the patient sitting in a wet adult diaper.

2 Normative references

The following documents are referred to in the text in such a way that some or all of their content constitutes requirements of this document. For dated references, only the edition cited applies. For undated references, the latest edition of the referenced document (including any amendments) applies.

ISO 16840-2:2018, *Wheelchair seating — Part 2: Determination of physical and mechanical characteristics of seat cushions intended to manage tissue integrity*

3 Terms and definitions

For the purposes of this document, the following terms and definitions apply.

ISO and IEC maintain terminology databases for use in standardization at the following addresses:

- ISO Online browsing platform: available at <https://www.iso.org/obp>
- IEC Electropedia: available at <https://www.electropedia.org/>

3.1

indenter ischial tuberosity

one of two locations on the inferior surface of an indenter that corresponds in position to the location of a human ischial tuberosity

3.2

electrical impedance

complex number ratio of the voltage to the current in an alternating current circuit

Note 1 to entry: Impedance extends the concept of electrical resistance to the alternating current circuit.

3.3

sensible perspiration

perspiration that has not gone through a phase change to the vapour phase

Note 1 to entry: This is perspiration that can be felt as being moist by a person, in contrast with the water vapour phase of perspiration, which is described as insensible.

4 Abbreviated terms

PRCLI perspiration rigid cushion loading indenter

RCLI rigid cushion loading indenter

5 Principle

Human sensible perspiration in the area between the cushion and buttocks has four possible states:

- a) existing in between a cushion and the buttock (such as with a sealed vinyl cover);
- b) dissipated into the cushion cover, but not into the cushion;
- c) dissipated more generally into both the cover and cushion;
- d) drawn away from the cover (which becomes dry) and into the cushion.

The dissipation behaviour of the cover/cushion system can be evaluated by measuring the changing impedance at a location of interest following a discharge of simulated liquid perspiration into the area between the rigid cushion loading indenter and the cushion. The test method employs delivery of solution that simulates sensible perspiration in a single bolus. This allows the rate of dissipation to be determined.

The testing system has four elements:

- a RCLI simulating temperature, weight, and shape in a loading buttock;
- a discharge system that releases a discrete amount of solution that simulates sensible perspiration;
- a measurement system of the changing impedance associated with changing solution concentration near the electrodes (indirectly indicating the absorption of the cover/cushion);
- a test environment of defined temperature and humidity.

6 Test apparatus

The following test apparatus shall be used.

6.1 Perspiration rigid cushion loading indenter

6.1.1 Shape of PRCLI

The PRCLI is formed from $4\text{ mm} \pm 1\text{ mm}$ polycarbonate sheet formed according to the specifications for a RCLI with the inner surface of the shell formed to match the contour specified in ISO 16840-2:2018, Annex A.

6.1.2 Temperature control on the PRCLI

The PRCLI shall include a means of maintaining the temperature at $35\text{ }^{\circ}\text{C} \pm 0,1\text{ }^{\circ}\text{C}$ in the inferior surface of the PRCLI.

6.1.3 Loading mechanism

The loading mechanism shall provide the means to load the cushion through the PRCLI with a vertical force of $500\text{ N} \pm 10\text{ N}$ in accordance with ISO 16840-2:2018.

6.1.4 Discharge mechanism

A system to discharge $10\text{ ml} \pm 1\text{ ml}$ of $0,01\%$ sodium chloride (NaCl) solution within one second from a hole $2\text{ mm} \pm 0,2\text{ mm}$ diameter (see [Figure 2](#)) located at the indenter ischial tuberosity of the PRCLI (see [Figure 1](#)).

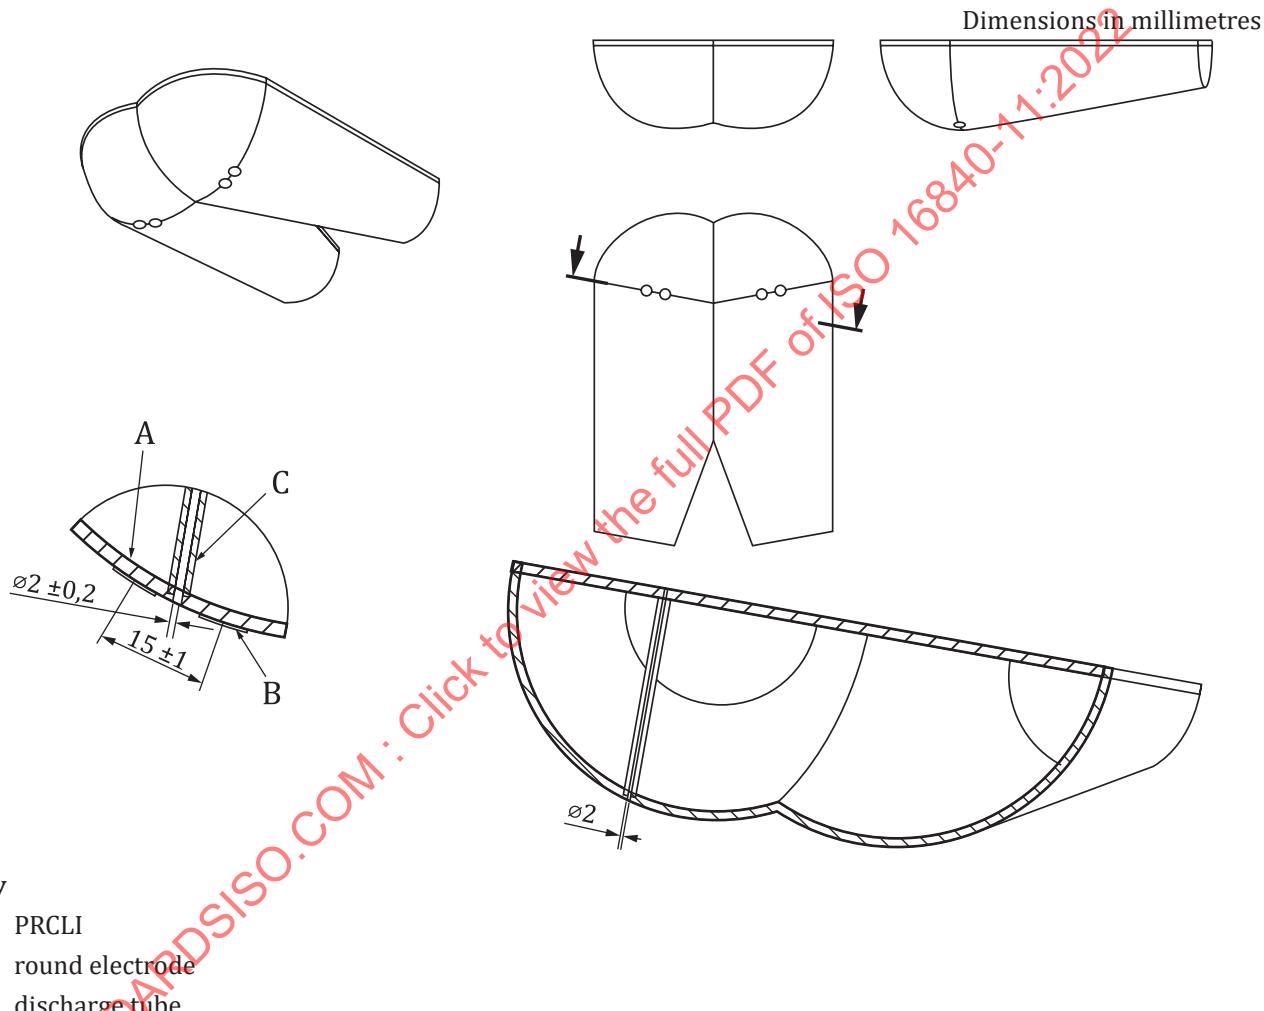
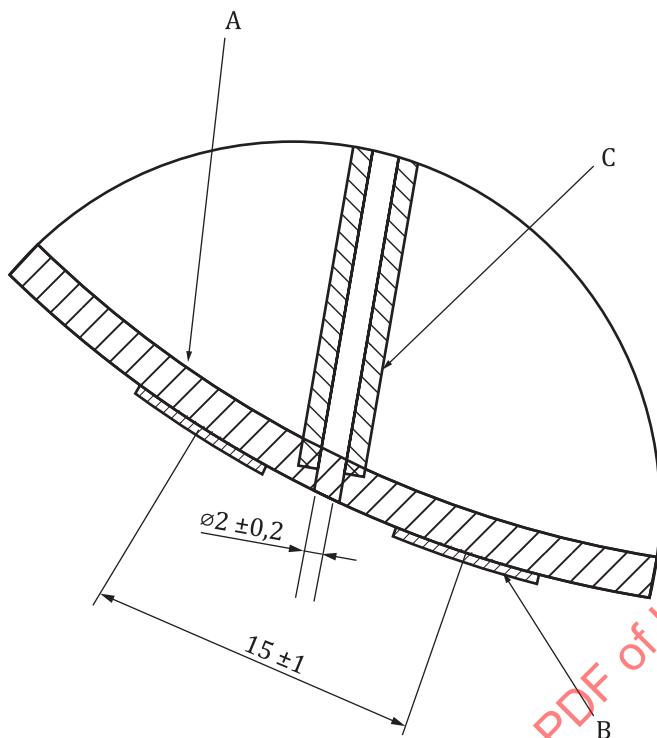


Figure 1 — Drawing of the PRCLI

Dimensions in millimetres

**Key**

- A PRCLI
- B round electrode
- C discharge tube

Figure 2 — Detail B from the A-B cross section of the PRCLI

6.1.5 Sensing system

The sensing system shall have a pair of equally sized round stainless steel electrodes. The electrodes shall be a thin plate with diameter of no less than 10 mm and no more than 15 mm, and a thickness of $0,1 \text{ mm} \pm 0,01 \text{ mm}$, preserving smoothness of the buttock surface. The centre of each electrode shall be $10 \text{ mm} \pm 1 \text{ mm}$ from the centre of the hole as shown in the cross-sectional diagram of the PRCLI (see [Figure 2](#)).

NOTE Stainless steel shim stock is normally acceptable for the electrodes.

6.2 Electrical impedance measurement system

An electrical impedance measurement system able to measure electrical impedance between the two electrodes, ranging from 0,001 MΩ to 1,0 MΩ, at a sampling rate of 1 Hz shall be used.

The electrodes shall be connected to the impedance measurement box external to the PRCLI by appropriately shielded electrical wires to minimize the electrical noise from the test environment. Alternating current should be selected for measurement to prevent electrolysis of the electrodes when in contact with the solution.

6.3 Test environment

A test environment shall be maintained at $23 \text{ }^{\circ}\text{C} \pm 2 \text{ }^{\circ}\text{C}$ and $50 \% \pm 5 \% \text{ relative humidity}$ (as specified in ISO 554) that includes the means to measure and record its temperature and humidity during the test period.

7 Preparation for testing

- 7.1 Select an unused cushion of 400 mm to 425 mm width and depth.
- 7.2 Select a cover that is unwashed or washed prior to testing. Either can be used.
- 7.3 Precondition the cushion to be tested by holding in the test environment of $23^{\circ}\text{C} \pm 2^{\circ}\text{C}$ and $50\% \pm 5\%$ relative humidity for 24 hours prior to test initiation.
- 7.4 Adjust the cushion per any manufacturer's instructions and test under those conditions. This can require testing in multiple stable states.
- 7.5 If indicated by the manufacturer, adjust the cushion to accommodate $500\text{ N} \pm 10\text{ N}$ load applied using the PRCLI

NOTE It will not be possible to run the test if the cover includes conductive elements that will shortcircuit the test electrodes.

8 Test method

- 8.1 Commence measurement of the impedance with a sampling rate of 1 Hz, with the PRCLI not in contact with the cushion/cover surface.
- 8.2 Apply a load of $500\text{ N} \pm 10\text{ N}$ to the cushion using the PRCLI.
- 8.3 Continue to record the impedance until at least $1\text{ h} \pm 1\text{ min}$ has elapsed from the commencement of the test. In some cases, change can be very slow and extended testing will be required.
- 8.4 After $1\text{ min} \pm 5\text{ sec}$, supply from the PRCLI to the cushion $10\text{ ml} \pm 1\text{ ml}$ of the NaCl solution from the tube within 1 sec.
- 8.5 Record the power required to maintain the PRCLI temperature at 35°C .
- 8.6 Repeat the testing on two further identical cushions.
- 8.7 Cushions with variable immersion settings should be tested at both the highest and lowest possible settings.

9 Test report

The test report shall contain the following:

- a) A reference to this document, i.e. ISO 16840-11:2022;
- b) The name and address of the testing institution;
- c) The accreditation status of the testing institution if any.
- d) The name and address of the manufacturer of the cushions;
- e) The date of issue and identification number of the test report;
- f) The test environment conditions as specified. If appropriate, this should include test conditions tested for in multiple stable states;

- g) The model type and nominal size that uniquely describes each test cushion and any cover that is used;
- h) A photograph of each test cushion with the cover prior to, during and following the test;
- i) The preparation of each test cushion and cover including whether or not the cover was washed or unwashed;
- j) A graph of the power required to maintain the PRCLI temperature at 35 °C as per [Clause 8](#) for each test.
- k) A graph of impedance values versus time for the period of the whole test as per [8.3](#) for each test.

NOTE See [Figure 3](#) for an example of the type of graph that can result.

- l) A table of the values of impedance for each test at
 - 1) the commencement of the test,
 - 2) immediately prior to the injection of the NaCl solution, and
 - 3) 12 min ± 20 sec intervals (from commencement of test) until the conclusion of the test.